

# **ABTS Antioxidant Assay Kit**

## **Cat# AOX-1**

### **STORAGE CONDITIONS**

All orders are delivered via Federal Express Priority courier at 4°C.  
All orders must be processed immediately upon arrival.

#### **ABTS Solution**

Store at 4°C.

#### **Trolox standard and Myoglobin reagent**

Store at -20°C

#### **Assay Buffer, Dilution Buffer, Stop Solution, and Assay Plate**

Store at room temperature

#### **Long-term storage:**

Remove the ABTS solution from the box and place at 4°C, store the Trolox and Myoglobin solutions at -20°C. Reagents are good for 3 months if stored properly.

#### **For *in vitro* Use Only**

#### **LIMITED PRODUCT WARRANTY**

This warranty limits our liability to replacement of this product. No other warranties of any kind, expressed or implied, including without limitation, implied warranties of merchantability or fitness for a particular purpose, are provided by Amsbio llc shall have no liability for any direct, indirect, consequential, or incidental damages arising out of the use, the results of use, or the inability to use this product.

The product accompanying this document is intended for research use only and is not intended for diagnostic purposes or for use in humans.


# TABLE OF CONTENTS

	<b><u>PAGE#</u></b>
Introduction	3
Principle of Assay	4
Items Included in the Kit	4
Sample Preparation	5
Assay Procedure	6
Trolox Standard Curve	7
Appendix : Plate layout	10
Appendix B: Protocol Flowchart	11
References	11

## INTRODUCTION

Free radicals and reactive oxygen species (ROS) are highly reactive molecules that are generated by normal cellular processes, environmental stresses, and UV irradiation. ROS react with cellular components, damaging DNA, carbohydrates, proteins, and lipids causing cellular and tissue injury. Excess production of reactive oxygen species can also lead to inflammation, premature aging disorders, and several disease states, including cancer, diabetes, and atherosclerosis. Organisms have developed complex antioxidant systems to protect themselves from oxidative stress, however, excess ROS can overwhelm the systems and cause severe damage.

The Zen-Bio ABTS Antioxidant Assay Kit can be used to determine the total antioxidant capacity of biological fluids, cells, and tissue. It can also be used to assay the antioxidant activity of naturally occurring or synthetic compounds for use as dietary supplements, topical protection, and therapeutics. The assay measures ABTS<sup>+</sup> radical cation formation induced by metmyoglobin and hydrogen peroxide. Trolox [6-Hydroxy-2,5,7,8-tetramethylchroman-2-carboxylic acid], a water soluble vitamin E analog, serves as a positive control inhibiting the formation of the radical cation in a dose dependent manner. The antioxidant activity in biological fluids, cells, tissues, and natural extracts can be normalized to equivalent Trolox units to quantify the composite antioxidant activity present. This assay measures radical scavenging by electron donation and when combined with Zen-Bio's ORAC antioxidant assay kit, provides a comprehensive analysis of a test sample's antioxidant activity

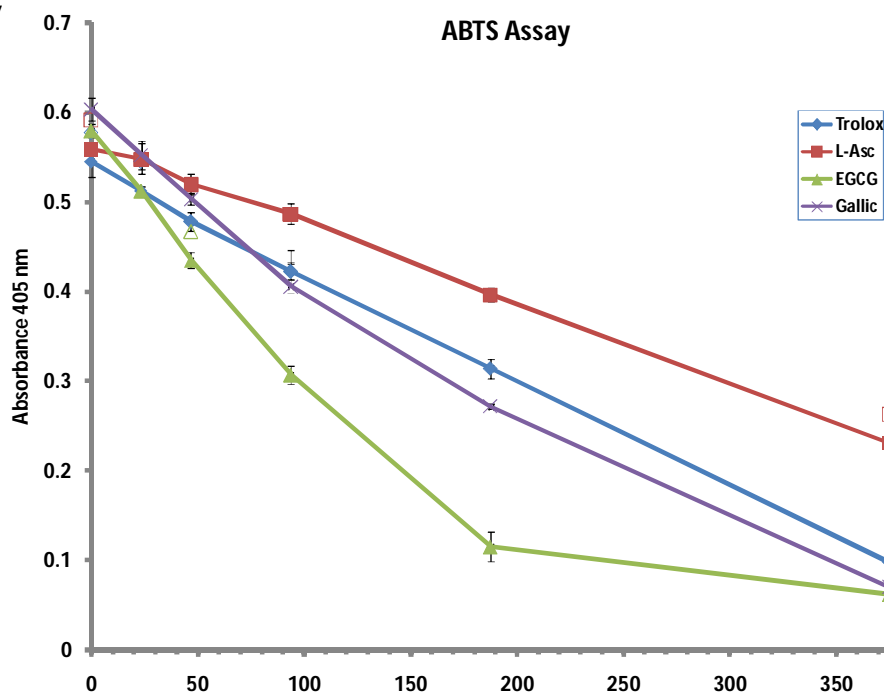

**Figure 1. Effects of antioxidants in ABTS assay**

Trolox, Sodium L-ascorbate (L-Asc), Epigallocatechin gallate (EGCG), and Gallic acid (Gallic) were tested for their antioxidant activity in the ABTS antioxidant assay.

## PRINCIPLE OF THE ASSAY

A ferryl myoglobin radical is formed from metmyoglobin and hydrogen peroxide. The ferryl myoglobin radical can oxidize ABTS (2,2'-azino-bis(3-ethylbenzthiazoline-6-sulfonic acid) to generate a radical cation,  $ABTS^{\cdot+}$ , that is green in color and can be measured by absorbance at 405nm. Antioxidants suppress this reaction by electron donation radical scavenging and inhibit the formation of the colored ABTS radical. The concentration of antioxidant in the test sample is inversely proportional to the ABTS radical formation and 405nm absorbance.



[Antioxidants inhibit the oxidation of ABTS by electron transfer radical scavenging]

## ITEMS INCLUDED IN THE KIT

ITEM	DESCRIPTION	Color	UNIT	QTY	STORAGE
Blank Assay Plates	96-well assay plates, blank	---	PLATE	1	-----
AOX Dilution Buffer	2.475 ml	AMBER	BOTTLE	1	RT
AOX Assay Buffer	11 ml	CLEAR	BOTTLE	1	RT
ABTS solution	11 ml	CLEAR	BOTTLE	1	4°C
Stop Solution	6ml	CLEAR	BOTTLE	1	RT
AOX Trolox	1.5mM in Dilution Buffer	AMBER	20 µl /VIAL	1	-20°C
Myoglobin Solution	100x stock	AMBER	30 µl /VIAL	1	-20°C
Tray	For multi-channel pipetters, clear polyvinyl	---	EACH	2	RT

**Other equipment/reagents required but not provided with the kit:**

- Multi-channel Pipet , single channel pipet and pipet tips
- Plate reader with a filter of 405 nm

### Reagents that might interfere with the assay results:

> 1% TWEEN 20	2-mercaptoethanol
> 1% TRITON X-100	Tris
IGEPAL CA-630 (Nonidet P-40)	Borate
> 0.2% CHAPS	DTT

# **SAMPLE PREPARATION**

---

## **Cell Lysate Preparation**

1. Scrape  $\sim 1 \times 10^6$  cells and centrifuge at 1,000xg to prepare a cell pellet. DO NOT use proteolytic enzymes such as trypsin but scrape using a rubber policeman or cell scraper tool.
2. Homogenize or sonicate the cell pellet on ice in 1ml cold AOX Assay buffer
3. Centrifuge at 10,000 x g for 15 minutes at 4°C.
4. Remove the supernatant and keep on ice until ready to use in the assay.
5. If not using the same day, store the samples at -80°C.
6. Data is expressed as Trolox equivalents (TE) per cell number (i.e.  $\mu\text{mole TE}/10^6$  cells)

## **Tissue Lysate Preparation**

1. Homogenize tissue samples on ice in cold buffer at  $\sim 200\text{mg}$  tissue per ml cold buffer
2. Centrifuge at 10,000 x g for 15 minutes at 4°C.
3. Remove the supernatant and keep on ice until ready to use in the assay.
4. If not using the same day, store the samples in small aliquots at -80°C.
5. Data is expressed as Trolox equivalents (TE) per gram of starting sample (i.e.  $\mu\text{M TE/g}$ )

## **Plasma Preparation**

1. Collect the blood in a tube containing heparin or other anticoagulant.
2. Centrifuge at 1,000 x g for 10 minutes at 4°C.
3. Remove the supernatant and keep on ice until ready to use in the assay.
4. If not using the same day, store the samples in small aliquots at -80°C.
5. Data is expressed as micromoles Trolox equivalents (TE) per volume sample (i.e.  $\mu\text{mole TE/L}$ )

## **Serum Preparation**

1. Collect the blood in a tube WITHOUT any anticoagulant. Allow the blood to clot.
2. Centrifuge at 2,000 x g for 10 minutes at 4°C.
3. Remove the supernatant and keep on ice until ready to use in the assay.
4. If not using the same day, store the samples in small aliquots at -80°C.
5. Data is expressed as micromoles Trolox equivalents (TE) per volume sample (i.e.  $\mu\text{mole TE/L}$ )

## **Saliva Collection**

1. Collect whole saliva for a defined period of time (i.e. 1-5 minutes) into polypropylene tubes.
2. Immediately place on ice or store at -80°C for later analysis.
3. Data is expressed as micromoles Trolox equivalents (TE) per volume sample (i.e.  $\mu\text{mole TE/L}$ )

## **Food Extract Preparation**


1. Weigh the starting material.
2. Homogenize in a small volume ice cold buffer or water.
3. Store small aliquots at -80°C for analysis.
4. When ready to assay, keep thawed samples on ice.
5. Data is expressed as Trolox equivalents (TE) per gram of starting sample (i.e.  $\mu\text{M TE/g}$ )

# ASSAY PROCEDURE

1. Remove the ABTS solution from the refrigerator and allow it to come to room temperature.

2. Prepare Trolox standards as follows:

Briefly spin down the contents of the 1.5 mM Trolox standard tube after thawing. Pipette 80  $\mu$ l of Assay Buffer into the 1.5 mM Trolox standard tube provided and mix well by vortexing. This produces a diluted stock Trolox standard of 300  $\mu$ M. Pipette 50  $\mu$ l of assay buffer into 6 tubes (not provided). Using the newly diluted stock Trolox solution, prepare a dilution series as depicted below. Mix each new dilution thoroughly before proceeding to the next. The 300  $\mu$ M stock dilution serves as the highest standard, and the assay buffer serves as the zero standard.

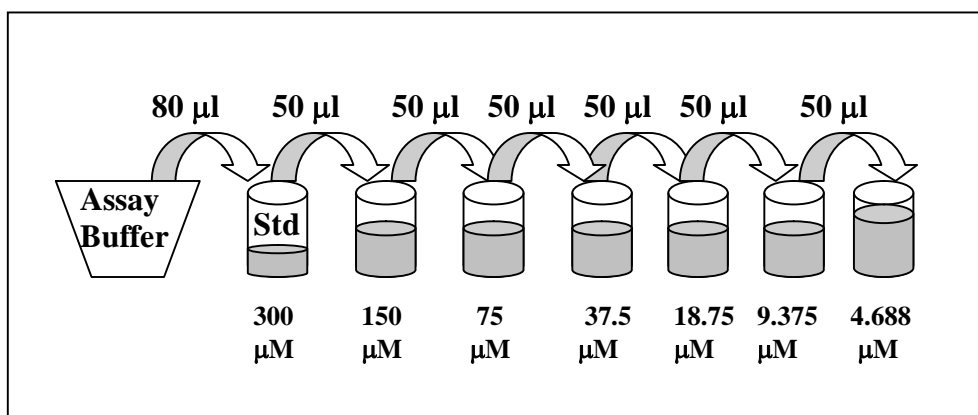

3. Prepare the Myoglobin Working Solution. Briefly spin down the contents of the Myoglobin stock solution tube. Add 25  $\mu$ l Myoglobin stock solution to the Dilution Buffer bottle (contains 2.475 ml) and gently invert. Place the working solution on ice until needed.

4. Add 10  $\mu$ l of samples or Trolox standards to individual wells of the assay plate provided, add 10  $\mu$ l of assay buffer to individual wells as a negative control.

5. Add 20  $\mu$ l of the myoglobin working solution to each of the wells containing standards and samples from step 4.

6. To begin the assay, add 100  $\mu$ l of the ABTS solution per well and place on plate shaker at room temperature. Allow the reaction to proceed for 5 minutes. To stop the reaction, add 50  $\mu$ l of Stop Solution per well.

7. Read absorbance using plate reader at a wavelength of 405 nm.


# TROLOX STANDARD CURVE

Generate standard curve: see example below

[DO NOT use this standard curve to generate your data. This is an example.]

$\mu\text{M}$ Trolox	OD	stdev
0	0.871	0.019
4.6875	0.864	0.006
9.375	0.855	0.003
18.75	0.829	0.018
37.5	0.806	0.006
75	0.742	0.013
150	0.636	0.009
300	0.436	0.013

slope =	-0.0015
intercept=	0.8629
$R^2$ =	0.9969

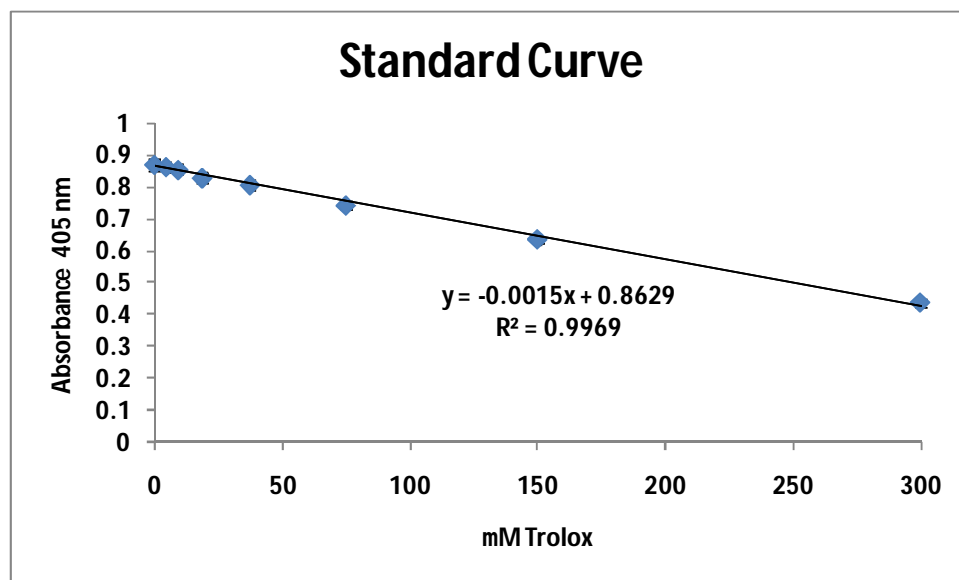

y = observed O.D.

x = concentration of Trolox in  $\mu\text{M}$

To calculate x for each y, (i.e. to change the observed O.D. into Trolox equivalent concentration) use the following equation:

y=(slope) times (x) plus intercept

$y=mx+b$  so  $x=(y-b)/m$

$x=(y - 0.8629)/(-.0015)$  where  $(-.0015)$ = slope of the line and  $0.8629$ = y intercept. Be careful to enter the proper sign for the y intercept value as it may be a negative number.

**The  $R^2$  value should be equal or greater then 0.98 for the standard curve to be valid. Any  $R^2$  values below 0.98, must have the standard curve run again.**

Antioxidant activity is expressed as  $\mu\text{M}$  Trolox equivalents (TE).

# OPTIONAL KINETIC ASSAY PROCEDURE

1. Prepare Trolox and myoglobin reagents as described above.
2. Set-up plate reader for kinetic reading mode:  
Total time = 10 minutes  
Interval = 30 seconds  
Absorbance= 405nm
3. Add 10 µl of samples or Trolox standards to individual wells of the assay plate provided, add 10 µl of assay buffer to individual wells as a negative control.
4. Add 20 µl of the myoglobin working solution to each of the wells containing standards and samples from step 3.
5. To begin the assay, add 100 µl of the ABTS solution per well and place in plate reader and begin reading absorbance using the kinetic mode.

## TROLOX KINETIC STANDARD CURVE

		Trolox concentration (µM)									
		1500	750	375	187.5	93.75	46.875	23.4375	0		
Time (min.)	0	0.059	0.058667	0.060333	0.062	0.059667	0.080333	0.109333	0.142		
	0.5	0.055667	0.056	0.058	0.059333	0.102667	0.159333	0.189667	0.219333		
	1	0.055667	0.056333	0.057333	0.076333	0.183333	0.238667	0.268667	0.3		
	1.5	0.055667	0.055667	0.057667	0.154667	0.262	0.318333	0.35	0.381333	AUC	
	2	0.055333	0.055667	0.058	0.233667	0.341667	0.398	0.431333	0.463	1500	1.668667
	2.5	0.056	0.056333	0.098333	0.314333	0.422667	0.478333	0.512667	0.545	750	5.160833
	3	0.056333	0.056667	0.175667	0.394667	0.503	0.558	0.592667	0.625333	375	11.34033
	3.5	0.056	0.056333	0.252	0.474	0.582	0.636667	0.672	0.704	187.5	15.309
	4	0.056667	0.056667	0.328667	0.554333	0.662	0.715333	0.751333	0.783	93.75	17.17033
	4.5	0.057	0.057	0.405667	0.634667	0.742	0.794	0.830667	0.862333	46.875	18.284
	5	0.056333	0.056667	0.483	0.715333	0.820667	0.871333	0.909333	0.941333	23.4375	19.01283
	5.5	0.056667	0.077667	0.563333	0.797667	0.900667	0.95	0.99	1.024	0	19.76167
	6	0.057333	0.154333	0.645	0.881333	0.981	1.032333	1.072	1.109		
	6.5	0.057333	0.233667	0.729	0.966667	1.063	1.116333	1.155667	1.196		
	7	0.057	0.313333	0.813	1.053	1.145333	1.201667	1.240667	1.283		
	7.5	0.057333	0.396667	0.899333	1.142333	1.230667	1.29	1.328	1.372333		
	8	0.058	0.481667	0.987667	1.233333	1.319333	1.380333	1.417667	1.462667		
	8.5	0.058333	0.567667	1.075667	1.325667	1.408667	1.470333	1.507333	1.553		
	9	0.058333	0.654667	1.164667	1.419	1.500333	1.562667	1.599	1.644		
	9.5	0.059	0.743	1.254667	1.512667	1.594333	1.656333	1.692	1.736333		
	10	0.059333	0.832333	1.346667	1.608	1.690667	1.751333	1.785667	1.829333		


Area under the curve (AUC)

$$AUC = 0.5 + f_0 + f_1 + \dots + f_{20} + (0.5 \cdot f_{21})$$


Where  $f_x$  = Abs value at time points 0 – 10 min



**Figure 2. Absorbance over time for Trolox standards**

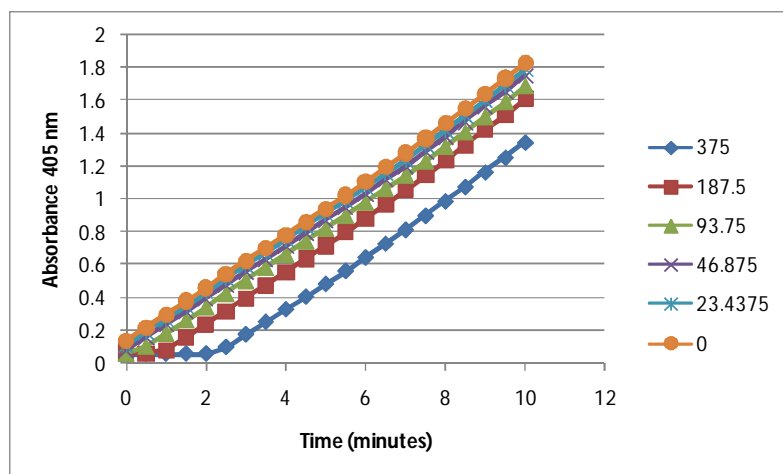


**Figure 3. AUC values for increasing Trolox concentrations**

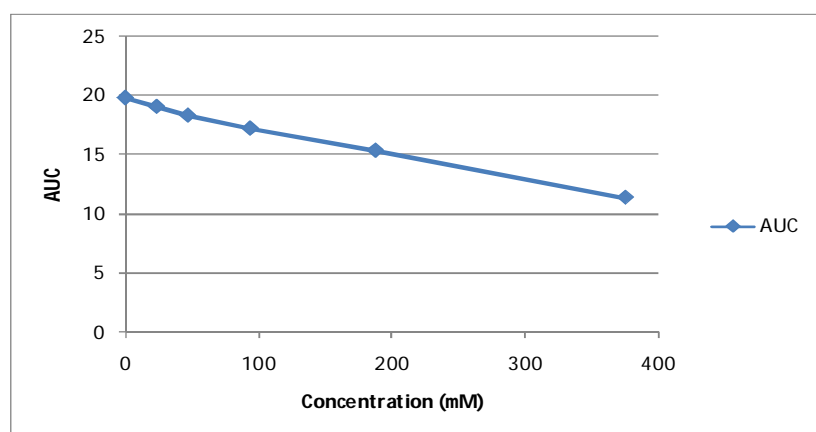


## Comparison of Stopped and Kinetic Assays

**Figure 4. ABTS Absorbance Values at 5 Minutes**

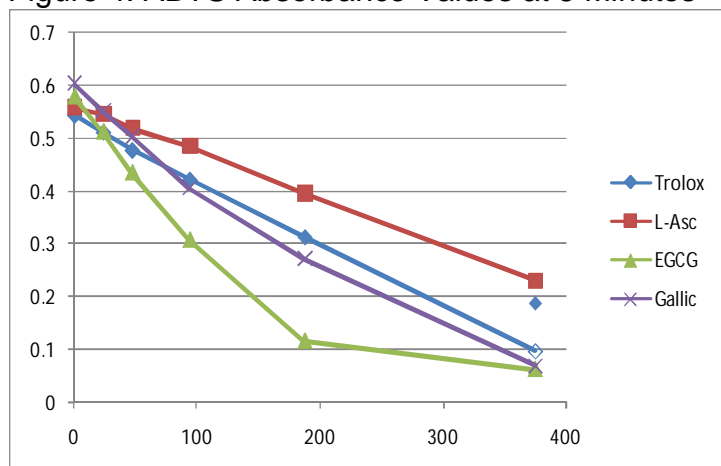

**Figure 5. AUC Values for Kinetic Assay**

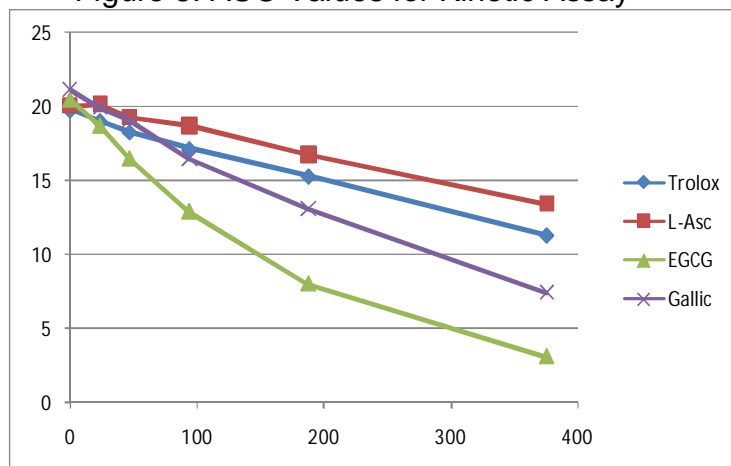

Trolox = Trolox [6-Hydroxy-2,5,7,8-tetramethylchroman-2-carboxylic acid]

L-Asc = Sodium L-ascorbate

EGCG = Epigallocatechin gallate


Gallic = Gallic acid

## APPENDIX A: Plate layout

	A	B	C	D	E	F	G	H
1								
2								
3								
4								
5								
6								
7								
8								
9								
10								
11								
12								

## APPENDIX B: Protocol Flowchart

### ABTS ASSAY

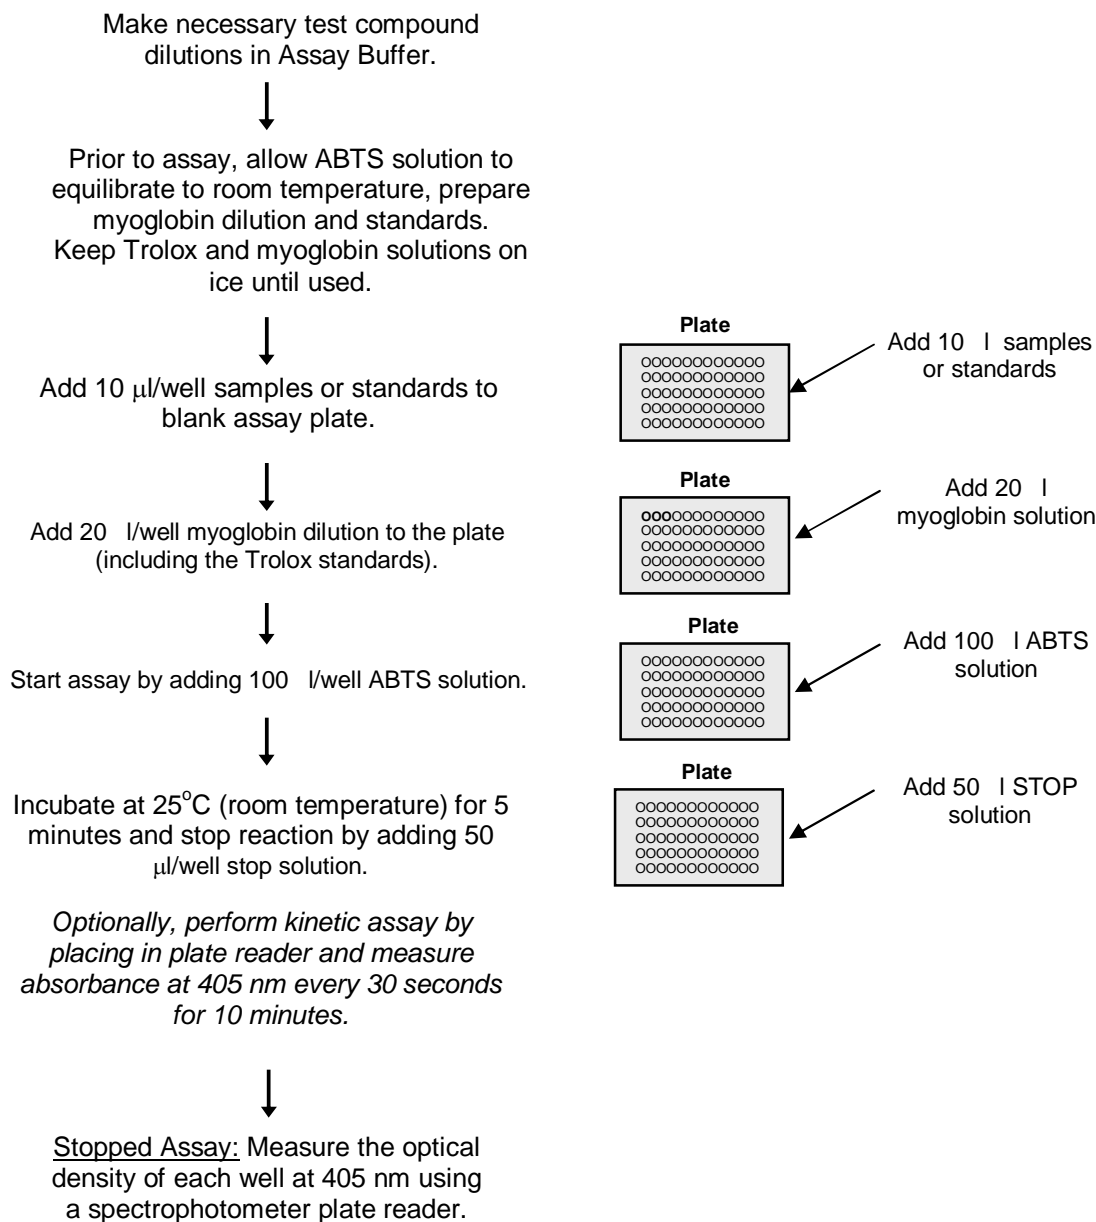

## REFERENCES

1. Clin. Chem., 44(6):1309–1315, 1998.
2. J. Clin. Biochem. Nutr., 44: 46–51, January 2009.
3. Indian J Biochem & Biophy. 46, 126-129 February 2009.



AMS BIOTECHNOLOGY (EUROPE) LTD  
UK & REST OF THE WORLD  
184 Park Drive, Milton Park  
Abingdon, OX14 4SE  
T: +44 (0) 1235 828 200  
F: +44 (0) 1235 820 482



AMSBIO LLC  
USA & CANADA  
1035 Cambridge Street,  
Cambridge, MA 02141  
T: +1 (617) 945-5033 or  
+1 (800) 987-0985  
F: +1 (617) 945-8218



AMS BIOTECHNOLOGY (EUROPE) LTD  
SWITZERLAND  
Via Lisano 3, (Cp.683)  
Ch-6900 Messagno  
T: +41 (0) 91 604 55 22  
F: +41 (0) 91 605 17 85



AMSBIO EUROPE BV  
EU  
Berenkoog 41,  
1822 BH Alkmaar,  
Netherlands  
T: +31 (0) 72 8080244  
F: +31 (0) 72 8080142