

Ferrous Iron Chelating (FIC) Assay Kit

Cat# AOX-15

INSTRUCTION MANUAL ZBM0124.00

STORAGE CONDITIONS

All orders are delivered via Federal Express Priority courier.
All orders must be processed immediately upon arrival.

All Reagents and Assay Plate

Store at room temperature

Long-term storage:

Reagents are good for at least 3 months after arrival if stored properly.

For *in vitro* Use Only

LIMITED PRODUCT WARRANTY

This warranty limits our liability to replacement of this product. No other warranties of any kind, expressed or implied, including without limitation, implied warranties of merchantability or fitness for a particular purpose, are provided by AMSBIO. AMSBIO shall have no liability for any direct, indirect, consequential, or incidental damages arising out of the use, the results of use, or the inability to use this product.

AMSBIO | www.amsbio.com | info@amsbio.com

UK & Rest of the World 
184 Park Drive, Milton Park
Abingdon OX14 4SE.
T: +44 (0) 1235 828 200
F: +44 (0) 1235 820 482

North America 
1035 Cambridge Street,
Cambridge, MA 02141.
T: +1 (617) 945-5033 or
T: +1 (800) 987-0985
F: +1 (617) 945-8218

Europe 
Berenkoog 41,
1822 BH Alkmaar,
Netherlands
T: +31 (0)72 8080244
F: +31 (0)72 8080142

Switzerland 
Via Lisano 3,
(CP.683)
CH-6900
T: +41 (0) 91 604 55 22
F: +41 (0) 91 605 17 85

Germany 
Bockenheimer Landstr. 17/19
60325 Frankfurt/Main
T: +49 (0) 69 779099
F: +49 (0) 69 13376880

TABLE OF CONTENTS

	<u>PAGE#</u>
Introduction	3
Principle of Assay	4
Items Included in the Kit	4
Assay Procedure	5
Data Analysis	6
Appendix : Plate layout	7
Appendix B: Protocol Flowchart	8
References	8
Frequently Asked Questions	9

AMSBIO | www.amsbio.com | info@amsbio.com

UK & Rest of the World 
184 Park Drive, Milton Park
Abingdon OX14 4SE.
T: +44 (0) 1235 828 200
F: +44 (0) 1235 820 482

North America 
1035 Cambridge Street,
Cambridge, MA 02141.
T: +1 (617) 945-5033 or
T: +1 (800) 987-0985
F: +1 (617) 945-8218

Europe 
Berenkoog 41,
1822 BH Alkmaar,
Netherlands
T: +31 (0)72 8080244
F: +31 (0)72 8080142

Switzerland 
Via Lisano 3,
(CP.683)
CH-6900
T: +41 (0) 91 604 55 22
F: +41 (0) 91 605 17 85

Germany 
Bockenheimer Landstr. 17/19
60325 Frankfurt/Main
T: +49 (0) 69 779099
F: +49 (0) 69 13376880

INTRODUCTION

Free radicals and reactive oxygen species (ROS) are highly reactive molecules that are generated by normal cellular processes, environmental stresses, and UV irradiation. ROS react with cellular components, damaging DNA, carbohydrates, proteins, and lipids causing cellular and tissue injury. Excess production of reactive oxygen species can also lead to inflammation, premature aging disorders, and several disease states, including cancer, diabetes, and atherosclerosis. Organisms have developed complex antioxidant systems to protect themselves from oxidative stress, however, excess ROS can overwhelm the systems and cause severe damage.

Excess transition metal ions, such as Fe(II), can generate hydroxyl radicals [OH•] in biological systems through Fenton-like reactions. Some antioxidants are able to chelate Fe(II) thereby inhibiting the formation of hydroxyl radicals and oxidative damage. The AMSBIO Ferrous Ion Chelating (FIC) Assay measures the capacity of test samples to chelate free ferrous ions in solution thereby inhibiting Fe(II) binding to ferrozine which generates a highly colored complex. EDTA serves as a positive control capable of chelating ferrous ions in a dose dependent manner. The FIC assay is an endpoint assay measuring absorbance of the ferrous-ferrozine complex at $\lambda = 562\text{nm}$. FIC activity is determined as the percent of total ferrozine / Fe(II) binding.

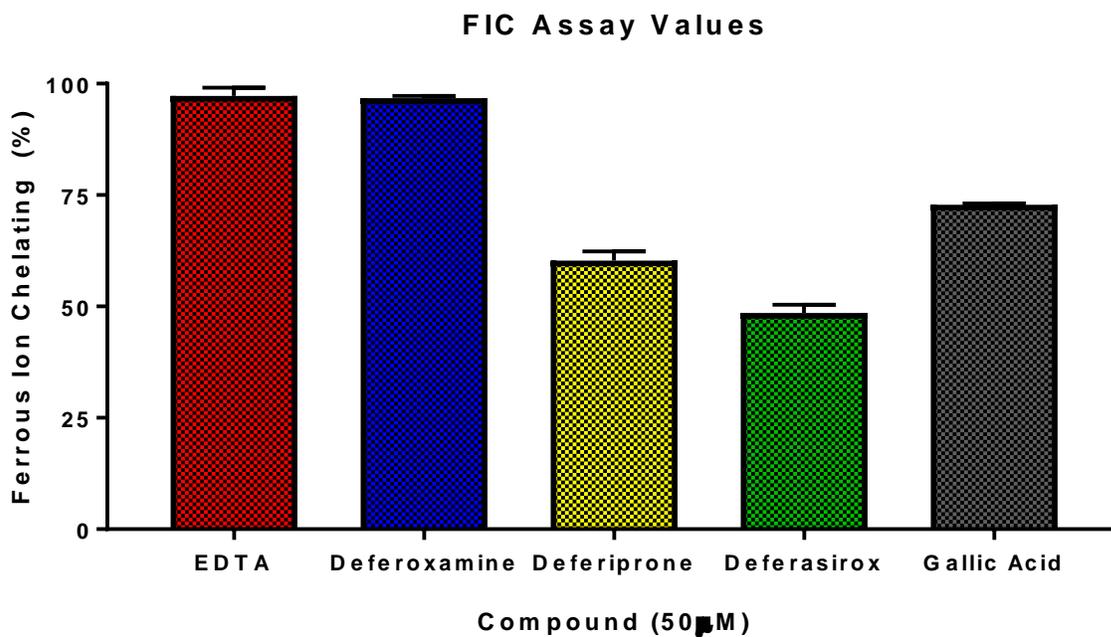


Figure 1. Fe(II) Chelating Activity of Compounds in the FIC Assay
 EDTA, Deferoxamine, Deferiprone, Deferasirox, and Gallic acid were tested at 50µM for their Fe(II) chelation activity in the FIC assay.

AMSBIO | www.amsbio.com | info@amsbio.com

UK & Rest of the World 184 Park Drive, Milton Park Abingdon OX14 4SE. T: +44 (0) 1235 828 200 F: +44 (0) 1235 820 482

North America 1035 Cambridge Street, Cambridge, MA 02141. T: +1 (617) 945-5033 or T: +1 (800) 987-0985 F: +1 (617) 945-8218


Europe Berenkoog 41, 1822 BH Alkmaar, Netherlands T: +31 (0)72 8080244 F: +31 (0)72 8080142

Switzerland Via Lisano 3, (CP.683) CH-6900 T: +41 (0) 91 604 55 22 F: +41 (0) 91 605 17 85

Germany Bockenheimer Landstr. 17/19 60325 Frankfurt/Main T: +49 (0) 69 779099 F: +49 (0) 69 13376880

PRINCIPLE OF THE ASSAY

Ferrozine (3-(2-Pyridyl)-5,6-diphenyl-1,2,4-triazinep,p'-disulfonic acid) is able to form a complex with free ferrous ions (Fe(II)) resulting in a chromophore with strong absorbance at 562nm. Compounds that are able to chelate Fe(II) lower the amount of free Fe(II) in solution, decreasing the Ferrozine-Fe(II) complex concentration, which results in a loss of absorbance at 562nm.



ITEMS INCLUDED IN THE KIT

ITEM	DESCRIPTION	Color	UNIT	QTY	STORAGE
Blank Assay Plates	96-well assay plates, blank	---	PLATE	2	-----
AOX Assay Buffer	30 ml	CLEAR	BOTTLE	1	RT
FeSO ₄ powder	5 mg	AMBER	VIAL	1	RT
Ferrozine powder	5 mg	CLEAR	BOTTLE	1	RT
EDTA solution	10mM in Assay Buffer	CLEAR	50 µl /VIAL	1	RT
Tray	For multi-channel pipetters, clear polyvinyl	---	EACH	2	RT

Other equipment/reagents required but not provided with the kit:

- Multi-channel Pipet , single channel pipet and pipet tips
- Tubes for preparing dilutions.
- Distilled water
- Plate reader with a filter of ~562 nm

Reagents that might interfere with the assay results:

EDTA and other strong iron chelators

AMSBIO | www.amsbio.com | info@amsbio.com

UK & Rest of the World 
184 Park Drive, Milton Park
Abingdon OX14 4SE.
T: +44 (0) 1235 828 200
F: +44 (0) 1235 820 482

North America 
1035 Cambridge Street,
Cambridge, MA 02141.
T: +1 (617) 945-5033 or
T: +1 (800) 987-0985
F: +1 (617) 945-8218

Europe 
Berenkoog 41,
1822 BH Alkmaar,
Netherlands
T: +31 (0)728080244
F: +31 (0)728080142

Switzerland 
Via Lisano 3,
(CP.683)
CH-6900
T: +41 (0) 91 604 55 22
F: +41 (0) 91 605 17 85

Germany 
Bockenheimer Landstr. 17/19
60325 Frankfurt/Main
T: +49 (0) 69 779099
F: +49 (0) 69 13376880

ASSAY PROCEDURE

1. Prepare 100x FeSO₄ Solution by adding 1.8mL of distilled water to the tube containing 5mg of FeSO₄. Mix by vortexing.
2. Prepare 100x Ferrozine Solution by adding 406µL of distilled water to the tube containing 5mg of Ferrozine. Mix by vortexing.
3. Prepare the 100 µM EDTA positive control in a separate tube by adding 10µL of the 10mM stock to 990µL of Assay Buffer.
4. Prepare test sample dilutions in Assay Buffer as necessary.
5. Make 6mL of Working FeSO₄ Solution by adding 60 µL of the 100x solution (from step 1) to 5.94mL of distilled water.
6. Add 50 µL of distilled water to three wells of the assay plate (background) and then add 50 µL of the Working FeSO₄ Solution to the remaining wells.
7. Add 50 µL of Assay Buffer to the 3 background wells containing distilled water from step 6.
8. Add 50 µL of Assay Buffer to an additional 3 wells for the maximal signal control.
9. Add 50 µL of samples and 100µM EDTA to triplicate wells.
10. Make 12mL of Working Ferrozine Solution by adding 120 µL of the 100x Ferrozine solution (from step 2) to 11.98mL distilled water and mix.
11. To begin the assay, add 100 µL of the Working Ferrozine Solution to each well of the assay plate and incubate at room temperature for 10 minutes.
12. Determine absorbance using plate reader at a wavelength of 562 nm.

ALTERNATIVE ASSAY PROCEDURE

This includes an EDTA standard curve to determine EDTA equivalents of test samples.

Prepare the EDTA standards according to the following table:

Standard	Final Conc. (µM)	Assay Buffer (µL)	Volume (µL)	EDTA Solution
Std100	100	0	300	100 µM solution
Std50	50	150	150	Std100
Std25	25	150	150	Std50
Std12.5	12.5	150	150	Std25
Std6.25	6.25	150	150	Std12.5
Std3.125	3.125	150	150	Std6.25
Std1.56	1.56	150	150	Std3.125
Std0	0	150	0	0

Mix each new dilution thoroughly before proceeding to the next step.

Add 50 µL of each standard to duplicate wells on each assay plate used.

DATA ANALYSIS

Values are determined as a percent Ferrous ion chelating (%).

1. Determine the background absorbance value by averaging the absorbance values of the three background wells (no FeSO₄ or sample).
2. Subtract the background absorbance from all of the absorbance values.
3. Determine the maximal absorbance value by averaging the absorbance values of the three wells containing FeSO₄, Ferrozine and Assay Buffer (from step 8, above).
4. Use the following equation to determine the ferrous ion chelating percent:

$$\text{Ferrous ion chelating (\%)} = 100 \times (\text{Abs}_{\text{max}} - \text{Abs}_{\text{test}}) / \text{Abs}_{\text{max}}$$

Abs_{max} is determined in step 3.

Abs_{test} is the absorbance of the test sample.


ALTERNATIVE DATA ANALYSIS

Values are determined as μM EDTA equivalents.

1. Determine Ferrous ion chelating (%) for all controls and samples as described above.
2. Plot EDTA concentration vs. Ferrous ion chelating (%).

EDTA uM	Chelating Activity (%)		Avg.	Stdev
100	101.04	100.94	100.9	0.07
33.33	95.90	95.39	95.6	0.36
11.11	92.06	90.6	91.3	0.99
3.703	71.10	67.67	69.3	2.42
1.234	42.27	38.94	40.6	2.35
0.411	22.71	17.87	20.2	3.42
0.137	17.37	17.57	17.4	0.14

This curve generated by 3-fold dilutions.

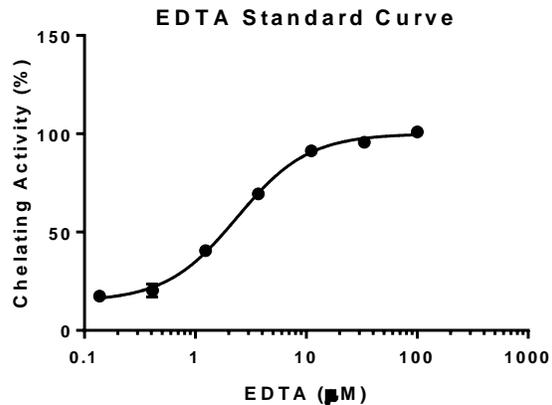

A three or four parameter fit may be applied to the data after log10 transforming the concentrations.

Use the values generated from your standard curve to back-calculate the equivalent EDTA concentration for each of your samples.

AMSBIO | www.amsbio.com | info@amsbio.com

UK & Rest of the World 184 Park Drive, Milton Park Abingdon OX14 4SE. T: +44 (0) 1235 828 200 F: +44 (0) 1235 820 482

North America 1035 Cambridge Street, Cambridge, MA 02141. T: +1 (617) 945-5033 or T: +1 (800) 987-0985 F: +1 (617) 945-8218

Europe Berenkoog 41, 1822 BH Alkmaar, Netherlands T: +31 (0)72 8080244 F: +31 (0)72 8080142

Switzerland Via Lisano 3, (CP.683) CH-6900 T: +41 (0) 91 604 55 22 F: +41 (0) 91 605 17 85

Germany Bockenheimer Landstr. 17/19 60325 Frankfurt/Main T: +49 (0) 69 779099 F: +49 (0) 69 13376880

APPENDIX A: Plate layout

H	G	F	E	D	C	B	A	
								1
								2
								3
								4
								5
								6
								7
								8
								9
								10
								11
								12

APPENDIX B: Protocol Flowchart

FERROUS IRON CHELATING ASSAY


Prior to assay, prepare working solutions of FeSO₄ and Ferrozine. Prepare EDTA positive control or alternatively, standard curve.




Make necessary test compound dilutions in Assay Buffer.




Add 50 µl/well Working FeSO₄ Solution to blank assay plate. Add 50 µl distilled water to triplicate wells for background.

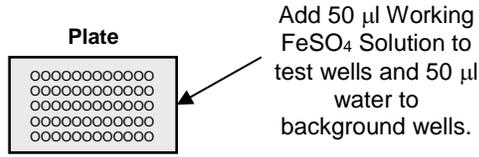

Add 50 µl/well samples or standards to assay plate.

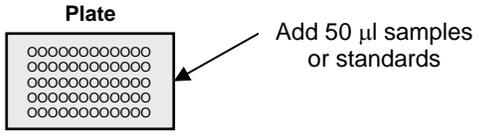

Start the assay by adding 100 µl/well Working Ferrozine Solution.

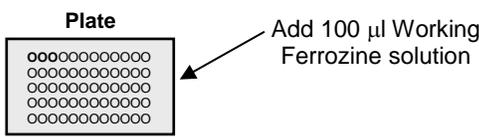

Incubate at 25°C (room temperature) for 10 minutes.



Measure the optical density of each well at 562 nm using a spectrophotometer plate reader.

REFERENCES

1. Int. J. Food Sci. Nutr., **56**(7):491–499, 2005.
2. Food Chem., **214**:515-522, 2017

AMSBIO | www.amsbio.com | info@amsbio.com

UK & Rest of the World 184 Park Drive, Milton Park Abingdon OX14 4SE. T: +44 (0) 1235 828 200 F: +44 (0) 1235 820 482

North America 1035 Cambridge Street, Cambridge, MA 02141. T: +1 (617) 945-5033 or T: +1 (800) 987-0985 F: +1 (617) 945-8218

Europe Berenkoog 41, 1822 BH Alkmaar, Netherlands T: +31 (0)72 8080244 F: +31 (0)72 8080142

Switzerland Via Lisano 3, (CP.683) CH-6900 T: +41 (0) 91 604 55 22 F: +41 (0) 91 605 17 85

Germany Bockenheimer Landstr. 17/19 60325 Frankfurt/Main T: +49 (0) 69 779099 F: +49 (0) 69 13376880

FREQUENTLY ASKED QUESTIONS

1. **Is it alright that my absorbance values are lower than those in the sample data?** Yes, the absorbance values may vary from different plate readers, however the background and maximum control values should be at least 0.1 absorbance units different.
2. **Should I dilute my sample for testing its FIC activity?** In order to accurately determine the FIC activity of your sample, it is likely necessary to prepare several dilutions to ensure that you generate a dose dependent response.

AMSBIO | www.amsbio.com | info@amsbio.com

UK & Rest of the World 
 184 Park Drive, Milton Park
 Abingdon OX14 4SE.
 T: +44 (0) 1235 828 200
 F: +44 (0) 1235 820 482

North America 
 1035 Cambridge Street,
 Cambridge, MA 02141.
 T: +1 (617) 945-5033 or
 T: +1 (800) 987-0985
 F: +1 (617) 945-8218

Europe 
 Berenkoog 41,
 1822 BH Alkmaar,
 Netherlands
 T: +31 (0)728080244
 F: +31 (0)728080142

Switzerland 
 Via Lisano 3,
 (CP.683)
 CH-6900
 T: +41 (0) 91 604 55 22
 F: +41 (0) 91 605 17 85

Germany 
 Bockenheimer Landstr. 17/19
 60325 Frankfurt/Main
 T: +49 (0) 69 779099
 F: +49 (0) 69 13376880