

Cultured Human Adipocyte Lipolysis Assay Kit

Non-Esterified Fatty Acids Detection

100 point assay kit

Cat# LIP-2; LIP-2-NC

INSTRUCTION MANUAL ZBM0010.04

STORAGE CONDITIONS

- **Human Adipocytes**

NOTE:


Domestic customers: Assay must be performed 5-7 days AFTER receipt.
International customers: Assay must be performed 3-5 days AFTER receipt

- **Reagents & Buffers:** 4°C
- **Vehicle & Controls:** -20°C
- **Assay plate A (96-well) cultured human adipocytes:** 37°C

All Zen-Bio Inc products are for research use only. Not approved for human or veterinary use or for use in diagnostic or clinical procedures.

LIMITED PRODUCT WARRANTY

This warranty limits our liability to replacement of this product. No other warranties of any kind, expressed or implied, including without limitation, implied warranties of merchantability or fitness for a particular purpose, are provided by Zen-Bio, Inc. Zen-Bio, Inc. shall have no liability for any direct, indirect, consequential, or incidental damages arising out of the use, the results of use, or the inability to use this product.



UK & Rest of World

184 Milton Park, Abingdon
OX14 4SE, Oxon, UK
Tel: +44 (0) 1235 828 200
Fax: +44 (0) 1235 820 482

Switzerland

Centro Nord-Sud 2E
CH-6934 Bioggio-Lugano
Tel: +41 (0) 91 604 55 22
Fax: +41 (0) 91 605 17 85

Deutschland

Bockenheimer Landstr. 17/19
60325 Frankfurt/Main
Tel: +49 (0) 69 779099
Fax: +49 (0) 69 13376880

United States

23591 El Toro Rd, Suite #167
Lake Forest, CA 92630
Tel: + 1 800 987 0985
Fax: + 1 949 265 7703


INTRODUCTION

Lipolysis plays a central role in the regulation of energy balance. Lipolysis is the process in which triglycerides are hydrolyzed into glycerol and free fatty acids. This process releases free fatty acids (FFA) into the bloodstream where they may be either re-esterified by the adipocyte or travel to other tissues and exert other effects throughout the body. Elevated adipocyte lipolysis has been observed in obese and diabetic individuals (Arner 1996). Alterations in lipolytic capacity have also been implicated in the susceptibility to obesity of African-American individuals versus their Caucasian cohorts (Danadian *et al.* 2001).

The sympathetic nervous system plays a key role in the regulation of lipid mobilization. The main lipolytic pathway involves beta-agonists (β -agonists), which activate β -adrenergic receptors via the intracellular G_s proteins in adipocytes. This leads to the activation of adenylyl cyclase (AC), which then increases cyclic AMP (cAMP) levels. Elevated cAMP acts as a second messenger to activate hormone sensitive lipase (HSL). HSL, the rate-limiting enzyme regulating adipocyte lipolysis, then catalyzes the hydrolysis of triglycerides and results in the release of glycerol and FFA (increased lipolysis). Phosphodiesterases (PDE) are enzymes that hydrolyze cAMP to 5'-AMP (5 prime adenosine monophosphate). This action results in a decrease in lipolysis. PDE inhibitors increase intracellular cAMP levels. 3-isobutyl-1-methylxanthine (IBMX), a non-specific inhibitor of cAMP phosphodiesterases (PDE), is used as the positive control if your test compounds are suspected PDE inhibitors. Isoproterenol, a non-specific β -adrenergic agonist is used as the positive control if your test compounds affect lipolysis via β -adrenergic receptors.

This lipolysis assay kit provides the tool to study chemical compounds that may influence lipolysis in cultured human adipocytes.

Figure 1. Overview of adipocyte lipolysis

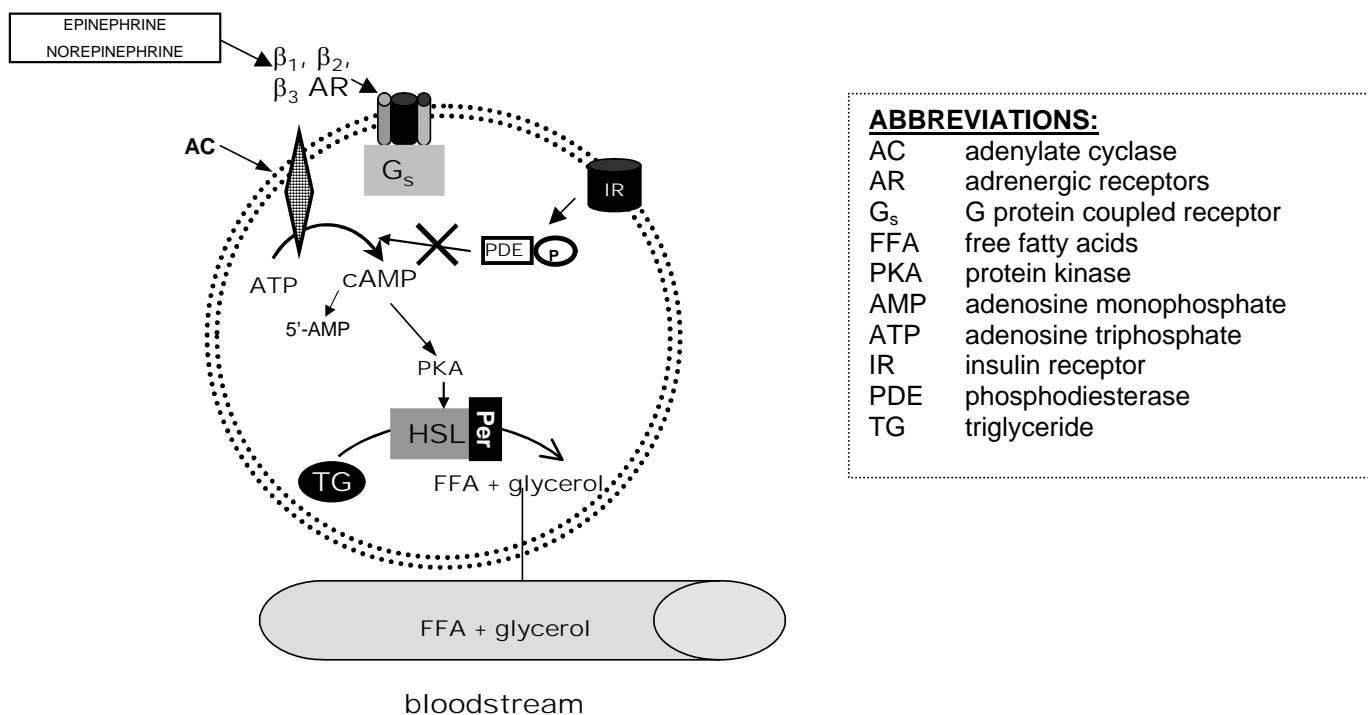

UK & Rest of World

184 Milton Park, Abingdon
OX14 4SE, Oxon, UK
Tel: +44 (0) 1235 828 200
Fax: +44 (0) 1235 820 482

Switzerland

Centro Nord-Sud 2E
CH-6934 Bioggio-Lugano
Tel: +41 (0) 91 604 55 22
Fax: +41 (0) 91 605 17 85

Deutschland

Bockenheimer Landstr. 17/19
60325 Frankfurt/Main
Tel: +49 (0) 69 779099
Fax: +49 (0) 69 13376880


United States

23591 El Toro Rd, Suite #167
Lake Forest, CA 92630
Tel: + 1 800 987 0985
Fax: + 1 949 265 7703

amsbio
info@amsbio.com

PRINCIPLE OF THE ASSAY

Assessment of lipolytic activity is through a coupled reaction to measure non-Esterified fatty acids (NEFA) released by adipocytes. The initial step, carried out by acyl-CoA synthetase (ACS), produces fatty acyl-CoA thiol esters from the NEFA, ATP, Mg, and CoA in the reaction. The acyl-CoA derivatives react with oxygen in the presence of acyl-CoA oxidase (ACOD) to produce hydrogen peroxide. Hydrogen peroxide in the presence of peroxidase (POD) allows the oxidative condensation of 3-methyl-N-ethyl-N-(β-hydroxyethyl)-aniline with 4-aminoantipyrine which forms a purple product that absorbs light at 550nm. This allows the concentration of NEFA to be determined from the optical density measured at 540 - 550nm.

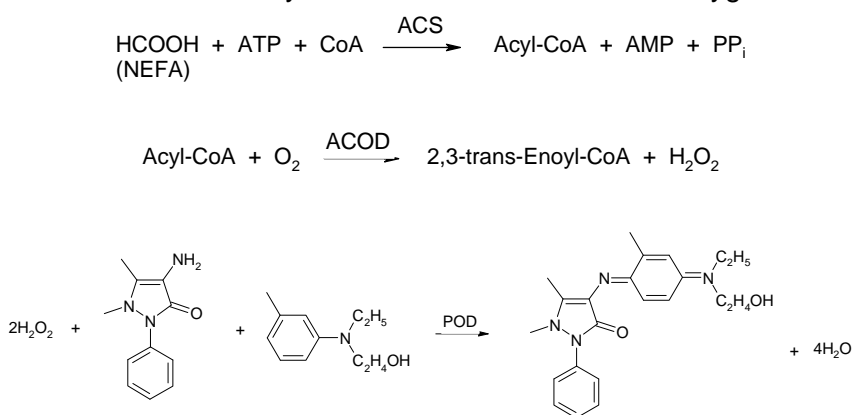


ITEMS INCLUDED IN THE KIT

ITEM	DESCRIPTION	Cap Color	UNIT	QTY	STORAGE
Adipocytes, Plate A	Cultured human subcutaneous adipocytes (LIP-2 only)	---	PLATE	1	37°C
Assay Plate	96-well assay plate, blank (for samples & standards)	---	PLATE	2	----
LIP-2/3 Assay Buffer	100 ml	---	BOTTLE	1	4°C
Wash Buffer	50 ml	---	BOTTLE	1	4°C
Vehicle	0.1% DMSO in LIP-2/3 Assay Buffer	PURPLE	1 ml / VIAL	1	-20°C
Positive control	Isoproterenol, 10 mM in DMSO. <u>Dilute to 1 μM in Assay Buffer before use!</u> (i.e. 1 μl in 10 ml Assay Buffer)	BLUE	10 μl / VIAL	1	-20°C
FFA Standard	1mM Stock. See page 5 for standard curve preparation	AMBER	100 μl / VIAL	1	4°C
FFA Diluent A		LABEL YELLOW	10.5ML	1	4°C
FFA Diluent B		LABEL PINK	5.5ML	1	4°C
FFA Reagent A	Reconstitute using 10.5 ml FFA Diluent A. Discard remainder after 10 days	LABEL YELLOW	BOTTLE	1	4°C
FFA Reagent B	Reconstitute using 5.5 ml FFA Diluent B. Discard remainder after 10 days	LABEL PINK	BOTTLE	1	4°C
Tray	For multi-channel pipettors, clear polyvinyl	CLEAR	EACH	2	----

Other equipment/reagents required but not provided with the kit:

- Multi-channel Pipet , single channel pipet and pipet tips
- Plate reader with a filter of 540 nm
- Incubator at 37°C
- Large gauge needle
- Tubes for dilution of standards



UK & Rest of World

184 Milton Park, Abingdon
OX14 4SE, Oxon, UK
Tel: +44 (0) 1235 828 200
Fax: +44 (0) 1235 820 482

Switzerland

Centro Nord-Sud 2E
CH-6934 Bioggio-Lugano
Tel: +41 (0) 91 604 55 22
Fax: +41 (0) 91 605 17 85

Deutschland

Bockenheimer Landstr. 17/19
60325 Frankfurt/Main
Tel: +49 (0) 69 779099
Fax: +49 (0) 69 13376880

United States


23591 El Toro Rd, Suite #167
Lake Forest, CA 92630
Tel: + 1 800 987 0985
Fax: + 1 949 265 7703

amsbio
info@amsbio.com

ASSAY PROCEDURE

1. Preadipocytes are plated in 96 well plates and allowed to differentiate under standard Zen-Bio differentiation conditions for 1 week. Upon arrival, remove 150µl of the shipping medium from each well and discard. Place the plate (Plate A) in your incubator for 5-7 days (3-5 days for international customers) to allow the cells to recover from the stress of shipping. To ensure optimal performance, **DO NOT** feed the cells fresh medium during this time. Please observe the cells under a microscope prior to performing the assay [see the photograph in the Certificate of Analysis for the lot # of Plate A].
2. Make your stock solution using whatever vehicle is appropriate for your test compounds. Dilute your stock solutions to their final concentration in LIP-2/3 Assay Buffer (100 ml is available). NOTE: if desired, maintain a constant concentration of solvent by preparing all compound dilutions in the highest concentration of that solvent. Dilute your controls in assay buffer. Prepare all vehicles as appropriate for your compounds, 0.1% DMSO has been included as the vehicle for the positive controls. Include the Assay Buffer alone as a vehicle control. PLEASE NOTE: ZEN-BIO DOES NOT RECOMMEND THE USE OF SOLVENTS AT CONCENTRATIONS ABOVE 1%.
3. Remove 120 µl medium from each well. Gently add 200 µl Wash Buffer to all wells. Remove 200 µl of the media and Wash Buffer from each well and replace with another 200 µl Wash Buffer.
4. Remove all the media and Wash Buffer from the cells from triplicate wells. Treat the cells with 75 µl of the test compounds resuspended in Assay Buffer three (3) wells at a time. Treat with the diluted Isoproterenol as positive control. Use the Assay Buffer alone as one of the vehicle controls. Please be sure to include both the vehicle provided in the kit and your vehicle (if your test compounds are not dissolved in DMSO). The assay should be performed in triplicate.
5. Incubate the plates at 37°C-humidified incubator for 3 hours (for time course experiments the longest time point recommended is 5 hours). Note: Treatment times longer than 3 hours will result in significant fatty acid reutilization by the adipocytes and may decrease signal relative to total lipolysis activity.
6. Prepare the standard curve using the STANDARD SOLUTION as follows:
Briefly spin down the contents of the free fatty acid standard tube. Standards are: 0, 1.4, 4.1, 12.3, 37, 111, and 333 µM fatty acid. Prepare as follows:

The kit standard solution is the 1.0 mM standard. Pipette 120 μ l of Assay Buffer into 6 tubes (not provided). Pipette 60 μ l of the FFA Standard Stock into a tube labeled 333 μ M. Prepare a dilution series as depicted below. Mix each new dilution thoroughly before proceeding to the next. The Assay Buffer alone serves as the zero standard.

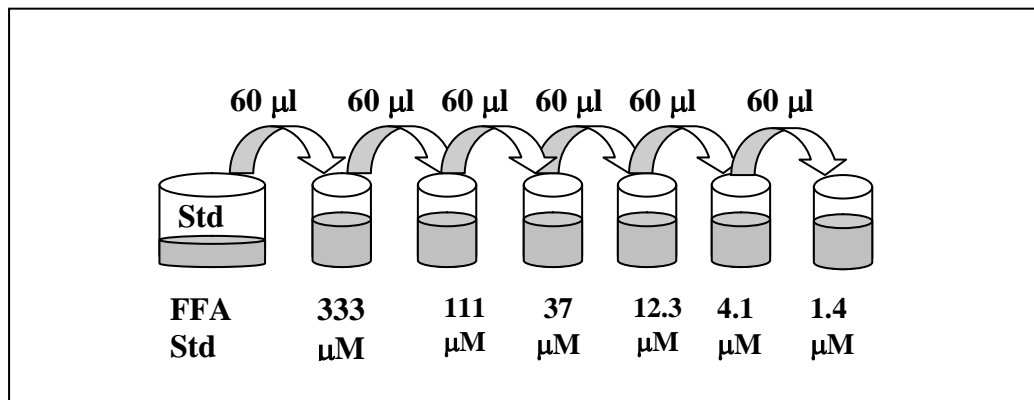

Note: The above dilution series generates enough volume to perform the standard curve in duplicate. If you wish to perform the standard curve in duplicate, please note that seven fewer data points can be assayed with this kit.

7. Add 10.5 ml FFA Diluent A to the FFA Reagent A bottle and gently invert. DO NOT VORTEX! Store any remaining solution at 2-8°C; it is stable for 10 days after reconstitution refrigerated (2-8°C).
8. At the end of the incubation, 50 μ l of the conditioned media is removed and transferred to the corresponding well of a blank plate for assessment of non-esterified fatty acids. [This is most easily accomplished using a multi-channel pipet.] Add 50 μ l of each standard to empty wells.
9. Add the reconstituted FFA Reagent A to one of the disposable trays provided in the kit. Add 100 μ l of FFA Reagent A to each well. Gently shake the plate to ensure mixing. Place in a 37 °C incubator for 10 minutes.
10. Add 5.5 ml FFA Diluent B to the FFA Reagent bottle and gently invert. Store any remaining solution at 2-8°C; it is stable for 10 days after reconstitution refrigerated (2-8°C).
11. Add the reconstituted FFA Reagent B to the other disposable tray provided in the kit. Add 50 μ l of FFA Reagent B to each well. Gently shake the plate to ensure mixing. Place in a 37 °C incubator for 10 minutes.

12. Allow the plate to equilibrate to room temperature for 5 minutes. During this time, ensure that there are no bubbles in the solution mixture. Use a large gauge needle or clean pipet tip to pop any bubbles as this will result in inaccurate absorbance readings.
13. The optical density of each well is then measured at 540 nm.


FATTY ACID STANDARD CURVE

Generate standard curve: see example below

[DO NOT use this standard curve to generate your data. This is an example.]

Subtract the OD value of the 0 μ M standard from all OD values including the standard curve. Note: 1mM standard is commonly omitted from analysis due to lack of linearity between 333 μ M and 1mM. Optionally, a 4-parameter fit may be used to calculate standard curve.

uM FFA	OD	OD	OD-blank	OD-blank	Avg OD-blank
0	0.05	0.048			0.049
1.4	0.051	0.053	0.002	0.004	0.003
4.1	0.056	0.058	0.007	0.009	0.008
12.3	0.070	0.075	0.021	0.026	0.024
37	0.119	0.122	0.070	0.073	0.072
111	0.274	0.277	0.225	0.228	0.227
333	0.689	0.750	0.640	0.701	0.671

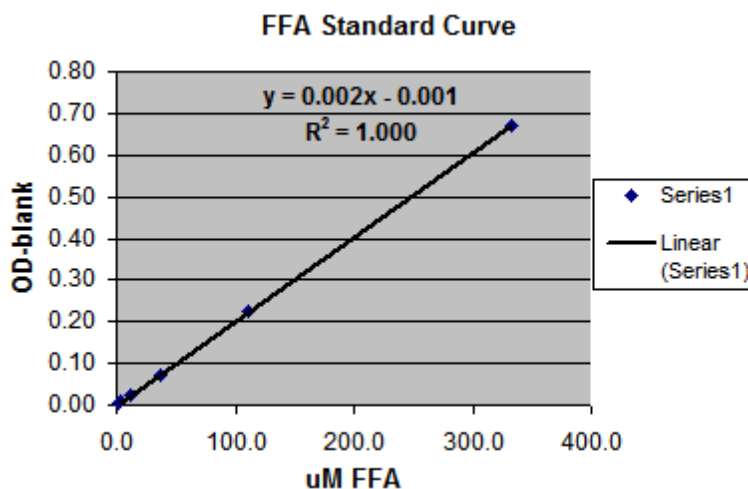

Slope	0.002
Intercept	-0.001
R ²	1.000

y = observed O.D. minus the blank

x = concentration of FFA in μ M

To calculate x for each y, (i.e. to change the observed O.D. into FFA concentration) use the following equation:

y=(slope) times (x) plus intercept

y=mx+b so $x=(y-b)/m$

$x=(y - (-0.001))/0.002$ where 0.002= slope of the line and -0.001= y intercept. Be careful to enter the proper sign for the y intercept value as it may be a negative number.

Data are expressed as μ M free fatty acids released.

OPTION: express data as Fold induction over appropriate vehicle

$$\text{Fold induction} = \frac{\mu\text{M free fatty acids SAMPLE}}{\mu\text{M free fatty acids VEHICLE}}$$

The R^2 value should be equal or greater than 0.98 for the standard curve to be valid. Any R^2 values below 0.98, must have the standard curve run again.

FREQUENTLY ASKED QUESTIONS

1. **I do not have time to run the assay. Can I freeze the conditioned media in PLATE B? How long can I store the samples before I complete the assay?** Yes. The conditioned media in PLATE B can be immediately stored at -80°C for a maximum of 7 days. Bring the conditioned media in PLATE B to room temperature BEFORE adding the FFA Reagents A and B and completing the assay.



UK & Rest of World

184 Milton Park, Abingdon
OX14 4SE, Oxon, UK
Tel: +44 (0) 1235 828 200
Fax: +44 (0) 1235 820 482

Switzerland

Centro Nord-Sud 2E
CH-6934 Bioggio-Lugano
Tel: +41 (0) 91 604 55 22
Fax: +41 (0) 91 605 17 85

Deutschland

Bockenheimer Landstr. 17/19
60325 Frankfurt/Main
Tel: +49 (0) 69 779099
Fax: +49 (0) 69 13376880

United States

23591 El Toro Rd, Suite #167
Lake Forest, CA 92630
Tel: + 1 800 987 0985
Fax: + 1 949 265 7703

amsbio
info@amsbio.com

APPENDIX A: PLATE LAYOUT

H	G	F	E	D	C	B	A	
								1
								2
								3
								4
								5
								6
								7
								8
								9
								10
								11
								12



UK & Rest of World
 184 Milton Park, Abingdon
 OX14 4SE, Oxon, UK
 Tel: +44 (0) 1235 828 200
 Fax: +44 (0) 1235 820 482

Switzerland
 Centro Nord-Sud 2E
 CH-6934 Bioggio-Lugano
 Tel: +41 (0) 91 604 55 22
 Fax: +41 (0) 91 605 17 85

Deutschland
 Bockenheimer Landstr. 17/19
 60325 Frankfurt/Main
 Tel: +49 (0) 69 779099
 Fax: +49 (0) 69 13376880

United States
 23591 El Toro Rd, Suite #167
 Lake Forest, CA 92630
 Tel: + 1 800 987 0985
 Fax: + 1 949 265 7703

amsbio
info@amsbio.com

APPENDIX B: LIP-2 PROCEDURE FLOWCHART

Remove 150µl of the shipping medium and place in your incubator for 5-7 days (3-5 days for international customers)



ON DAY OF ASSAY

Make all test compound dilutions in Assay Buffer.



Remove 120 µl media from all wells. Add 200 µl Wash Buffer to all wells.



Remove 120 µl media & Wash Buffer. Add another 200 µl Wash Buffer to all wells.



Remove all media & Wash Buffer. Add 75 µl treatments/controls to 3 wells at a time.



Incubate 3-5 hours at 37°C.



Remove 50 µl/well conditioned media from Plate A to one of the blank assay plates provided



Reconstitute FFA Reagent A using Diluent A. Add 100µl/well. Incubate 10 minutes @ 37°C.





Reconstitute FFA Reagent B using Diluent B. Add 50µl/well. Incubate 10 minutes @ 37°C.




Place at room temp. for 5 minutes. Pop any bubbles in each well using a clean pipet tip or large gauge needle.



Measure the optical density of each well at 540 nm using a spectrophotometer plate reader.

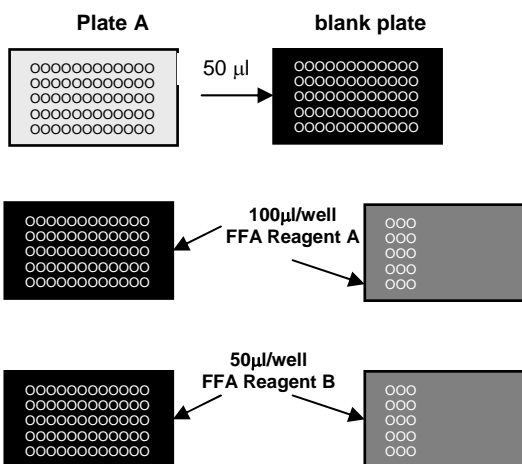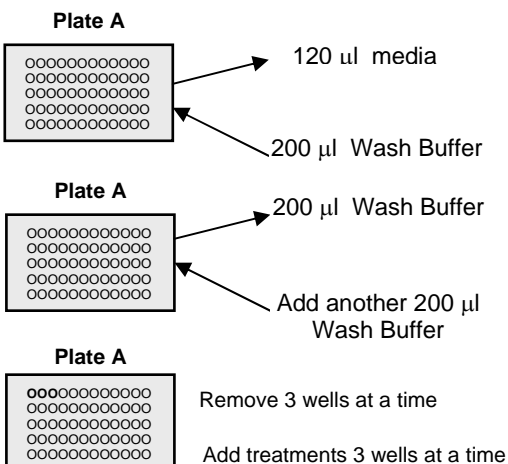

An additional plate may be necessary for the assay of standards.



UK & Rest of World

184 Milton Park, Abingdon
OX14 4SE, Oxon, UK
Tel: +44 (0) 1235 828 200
Fax: +44 (0) 1235 820 482

Switzerland

Centro Nord-Sud 2E
CH-6934 Bioggio-Lugano
Tel: +41 (0) 91 604 55 22
Fax: +41 (0) 91 605 17 85

Deutschland

Bockenheimer Landstr. 17/19
60325 Frankfurt/Main
Tel: +49 (0) 69 779099
Fax: +49 (0) 69 13376880

United States

23591 El Toro Rd, Suite #167
Lake Forest, CA 92630
Tel: + 1 800 987 0985
Fax: + 1 949 265 7703

amsbio
info@amsbio.com